References

- 1. Engineering data on file
- 2. Test report Evaluation of the microbial barrier performance of Caresite[®] valve against sporesog Bacillussubtilis signed by Prof. Dr. med. M.Exner and Dr. rer. nat. J. Gebel, Report DMT 2013-412. 11.12.2013
- 3. Test report Evaluation of the microbial barrier performance of the female valve Caresite® by touch contamination with Staphylococcus aureus signed by Prof. Dr. med. M.Exner and Dr. rer. nat. J. Gebel, Report DMT 2014-194, 09.12.2014
- 4. Test Report Closed system test by means of Sodium Fluorescein signed by Dr. rer. nat. J. Brünke Quality Labs BT GmbH Nuremberg, Report 1678.2-1, 28.05.2013
- 5. Choosing the Best Design for Intravenous Needleless Connectors to Prevent Bloodstream Infections written by William R. Jarvis, 28.07.2010
- 6. American Nurses Association Independent Study Module: Needlestick Safety and Prevention written by Mary Foley, MS, RN and Annemarie T. Leyden, EdD, RN
- 7. Review Article Review on Needle Free Drug Delivery Systems, International Journal of Pharma Research & Review, written by Bhagyashri Chavan, Abha Doshi, Yashwant Malode, Balu Misal, Sept 2013; 2(9):30-36

- 8. Engineering data on file: Caresite 7 Day Stress Cracking Lipids with Isopropanol
- 9. White Paper: CARESITETM Luer Access Device: Blood Clearance Test of the Needleless Connector, B. Braun Medical Inc., Bethlehem, PA., CS05 07/10 EB, 2010
- 10. White Paper: CARESITETM Luer Access Device: Mechanical Hemolysis Test of the Needleless Connector, B. Braun Medical Inc., Bethlehem, PA., CS06 07/10 EB. 2010
- 11. White Paper: CARESITE[®] Luer Access Device (LAD): 7- Day Microbial Barrier Performance, B. Braun Medical Inc., Bethlehem, PA., 15-5669 SW, 2017
- 12. Guidelines: Infusion Therapy Standards of Practice, page 152 published in Journal of Infusion Nursing (January/February 2016, Volume 39, Number 1S)
- 13. Study: Efficacy of a "saline only" flush protocol utilizing the Ultrasite® positive displacement device. Susan Silverstein, RN, CRNI, Nurse Consultant, Omnicare Infusion Services of Northern Illinois, January 2003
- 14. Study: Journal of Vascular Access Devices, Volume 5, Issue 4, 2000, Page 31-33, The effects of positive pressure devices on catheter occlusions, Loretta Berger RN, CRNI 15. Engineering data on file.



Caresite[®] Luer Access Device

B. Braun Melsungen AG | Hospital Care | 34209 Melsungen | Germany Tel. +49 5661 71-0 | www.bbraun.com



For more information, please scan the QR-code or visit: www.bbraun.com/en/products-and-therapies/b-braun-for-safety.html

Date of last revision: 07.2019







Needle-free access for Infusion Therapy

Caresite[®] Luer Access Device

Needle-free Luer Access Device with positive displacement feature


Caresite [®] Luer Access Device Performance Data ¹		Product features (all Caresite [®] configu	CLOSED	
 Fluid Displacement 	0.03 ml (positive)	Closed System ^{2, 3, 4, 5}	\checkmark	SYSTEM
 Durability (# accesses tested) 	1000	Needle-free System ^{6, 7}	\checkmark	
Only for Luer Access Device (straight valve*):		 Split septum valve technology 	, v	
 Flow rate 	208 ml/min	 Latex-free, DEHP-free 		
 Pressure resistance 	up to 400 psi @ 15 ml/sec		\checkmark	
Low priming volume**	0.22 ml	 Blood / Lipid compatible^{8, 9, 10} 	\checkmark	
Low retained volume**	0.20 ml	Luer-Lock / Luer-Slip compatible	\checkmark	

Product benefits



Helps to reduce microbial and chemical contamination^{2,3,4,11}

- Swabbable valve forms a closed system as it is designed to prevent microbial ingress and the escape of contaminants^{2,3}
- Smooth, swabbable surface (easy to clean)^{3,11}
- Clear design (easy to visually inspect)
- Self sealing valve helps to prevent spillage and drug exposure⁴

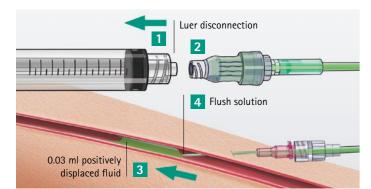



Designed to reduce the risk of catheter occlusion^{1, 12, 13, 14}

- Positive displacement (valve design)
- 1 Luer disconnection
- 2 Valve is closing automatically
- 3 0.03 ml positively displaced fluid
- 4 Flush solution inside the catheter tip

Ease of use

- High pressure resistant, suitable for use with power injectors* which allows more flexibility
- Ergonomic design provides easy access by allowing a good grip and easy connection¹⁵
- Drug compatible, tested with blood and lipids

Caresite®	Description	Length (cm)	Priming volume (ml)	Tubing inner ø (mm)	Units (pcs.)	Code No. (REF)
	Luer Access Device (high pressure resistant up to 400 psi for power injectors)	-	0.22	-	200/100****	415122-01
Caresite [®] extension	n sets					
	Smallbore extension set with Caresite [®] , Spin-Lock (high pressure resistant up to 300 psi for power injectors)	20	0.5	1.3	100	470100-01
	Standard bore extension set with Caresite [®] , Spin-Lock	15	0.9	2.8	100	470108-01
-70	Bifurcated smallbore extension set with 2 Caresite®, Spin-Lock	18	0.9	1.3	50	470106-01
T	Smallbore double extension set with 2 Caresite [®] , 2 back-check valves, Spin-Lock	22	1.6	1.3	100	470182
7	Smallbore triple extension set with 3 Caresite [®] , Spin-Lock	20	1.3	1.3	50	470160
-	Smallbore triple extension set with 3 Caresite [®] , 3 back-check valves, Spin-Lock	22	2.0	1.3	50	470161
	Standard bore extension set with female and male Luer-Lock connectors, back-check valve, and Caresite [®] 10 cm above distal end	23	1.5	2.8	50	470183
IV administration	sets with Caresite®					
	Intrafix [®] Primeline with Caresite [®]	180	20.5	3.0	100	40621580
	Intrafix [®] SafeSet with Caresite [®]	210	22.6	3.0	100	4063004C
	Intrafix® SafeSet Type Flush	180	22.0	3.0	25	4110000

* REF 415122-01 and 470100-01, ** compared to other positive displacement Luer Access Devices

**** dispenser box